



## Testing for blood glucose




### Removing the test strip

Push a test strip upwards with slight pressure from the front or back. With this test strip you can also touch the upper side.



### Inserting a test strip

Insert the test strip into the test strip slot in the direction of the arrow. If you switch on the device beforehand, you will automatically activate illumination.

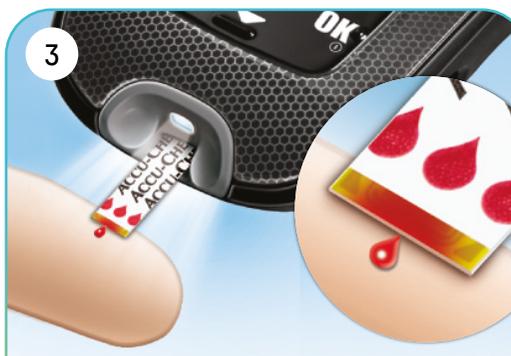

### Applying blood

Touch the drop of blood with the yellow edge of the test strip and wait until the "Measurement in progress" message appears.



### Ejecting the test strip

Remove the test strip by activating the test strip ejector button or by pulling the test strip out.

## Preparation

Insert lancet drum



- 1 Remove cap
- 2 Insert drum
- 3 Replace cap




Rotate the cap until the marking shows the desired penetration depth.

## Obtaining blood

Just 1 click!

Only  
1 click  
for priming and  
triggering

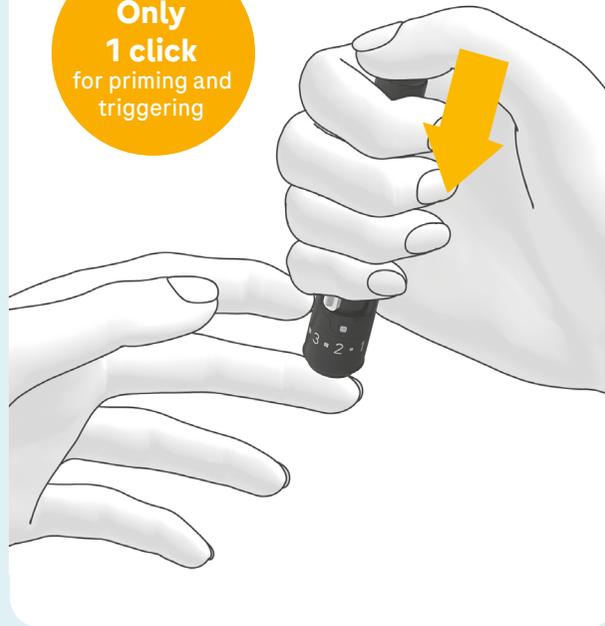

Press release button down completely to take a blood sample.

## Next step

Preparing and removing the lancet drum



- 1 First turn lever downwards to stop, then back in upwards direction.
- 2 For removal, pull off cap and pull out the drum.

Unused drum



Used drum



**Attention:** do not remove the lancet drum until all the lancets have been used. Once removed, the drum cannot be reinserted for hygienic reasons.